



EL879969365US



INVESTOR IN PEOPLE

The Patent Office
Concept House
Cardiff Road
Newport
South Wales
NP10 8QQ



I, the undersigned, being an officer duly authorised in accordance with Section 74(1) and (4) of the Deregulation and Contracting Out Act 1994, to sign and issue certificates on behalf of the Comptroller-General, hereby certify that annexed hereto is a true copy of the documents as originally filed in connection with the patent application identified therein together with the Statement of inventorship and of right to grant of a Patent (Form 7/77), which was subsequently filed.

In accordance with the Patents (Companies Re-registration) Rules 1982, if a company named in this certificate and any accompanying documents has re-registered under the Companies Act 1980 with the same name as that with which it was registered immediately before re-registration save for the substitution as, or inclusion as, the last part of the name of the words "public limited company" or their equivalents in Welsh, references to the name of the company in this certificate and any accompanying documents shall be treated as references to the name with which it is so re-registered.

In accordance with the rules, the words "public limited company" may be replaced by p.l.c., plc, P.L.C. or PLC.


Re-registration under the Companies Act does not constitute a new legal entity but merely subjects the company to certain additional company law rules.

Signed

Dated

18 June 2001



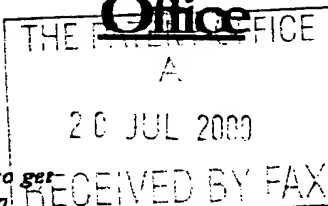

Request for grant of a patent

(See the notes on the back of this form. You can also get an explanatory leaflet from the Patent Office to help you fill in this form)

The Patent Office

Cardiff Road
Newport
Gwent NP9 1RH

1.	Your reference	P2636.A4/PAG		
2.	Patent application number (The Patent Office will fill in this part)	0017737.8		20 JUL 2000
3.	Full name, address and postcode of the or of each applicant (underline all surnames)	Hypoguard Limited Dock Lane Melton Woodbridge Suffolk IP12 1PE United Kingdom		
	Patents ADP number (if you know it)			
	If the applicant is a corporate body, give the country/state of its incorporation	4135 9 COR1		
4.	Title of the invention	TEST DEVICE		
5.	Name of your agent (if you have one)	DUMMETT COPP		
	"Address for service" in the United Kingdom to which all correspondence should be sent (including the postcode)	25 THE SQUARE MARTLESHAM HEATH IPSWICH IP5 3SL		
	Patents ADP number (if you know it)	6379001		
6.	If you are declaring priority from one or more earlier patent applications, give the country and the date of filing of the or of each of these earlier applications and (if you know it) the or each application number	Country	Priority application number (if you know it)	Date of filing (day / month / year)
7.	If this application is divided or otherwise derived from an earlier UK application, give the number and the filing date of the earlier application	Number of earlier application	Date of filing (day / month / year)	
8.	Is a statement of inventorship and of right to grant of a patent required in support of this request? (Answer 'Yes' if: a) any applicant named in part 3 is not an inventor, or b) there is an inventor who is not named as an applicant, or c) any named applicant is a corporate body. See note (d))	YES		

Patents Form 1/77

9. Enter the number of sheets for any of the following items you are filing with this form. Do not count copies of the same document

Continuation sheets of this form
THE PATENT OFFICE
A
20 JUL 2000
RECEIVED BY FAX

Description 15
Claim(s) 4
Abstract 1
Drawing(s) 11

10. If you are also filing any of the following, state how many against each item.

Priority documents

Translation of priority documents

Statement of inventorship and right to grant of a patent (Patents Form 7/77)

Request for preliminary examination and search (Patents Form 9/77) 1

Request for substantive examination (Patents Form 10/77) 1

Any other documents (please specify)

11. I/We request the grant of a patent on the basis of this application.

Signature

Date

DUMMETT COPP

20 July 2000

12. Name and daytime telephone number of person to contact in the United Kingdom
Dr Peter A Gemmell
01473 660600

Warning

After an application for a patent has been filed, the Comptroller of the Patent Office will consider whether publication or communication of the invention should be prohibited or restricted under Section 22 of the Patents Act 1977. You will be informed if it is necessary to prohibit or restrict your invention in this way. Furthermore, if you live in the United Kingdom, Section 23 of the Patents Act 1977 stops you from applying for a patent abroad without first getting written permission from the Patent Office unless an application has been filed at least 6 weeks beforehand in the United Kingdom for a patent for the same invention and either no direction prohibiting publication or communication has been given, or any such direction has been revoked.

Notes

- a) If you need help to fill in this form or you have any questions, please contact the Patent Office on 0645 500505.
- b) Write your answers in capital letters using black ink or you may type them.
- c) If there is not enough space for all the relevant details on any part of this form, please continue on a separate sheet of paper and write "see continuation sheet" in the relevant part(s). Any continuation sheet should be attached to this form.
- d) If you have answered 'Yes' Patents Form 7/77 will need to be filed.
- e) Once you have filled in the form you must remember to sign and date it.
- f) For details of the fee and ways to pay please contact the Patent Office.

Patents Form 1/77

TEST DEVICE

BACKGROUND OF THE INVENTION

5 1. Field of the Invention

The present invention relates to a test device for measuring the concentration of an analyte in a fluid sample, notably to a test device for analysing blood
10 glucose or other analytes in bodily fluids.

2. Description of the Prior Art

Diabetics regularly need to test samples of their blood to
15 determine the level of blood glucose. The results of such tests may be used to determine levels of medication needed to treat the diabetes at the time. In one known type of system, disposable sensors are used to test the blood. The sensors typically take the form of test strips which
20 are provided with a reagent material that will react with blood glucose to produce an electrical signal. Conductive tracks on the test strip relay the electrical signal to a meter which displays the result. After a sample of blood has been applied to the test strip and the measurement has
25 been taken, the test strip is disposed of. In order to couple the conductive tracks on a test strip with the meter, the test strip needs to be inserted into a sensor holder prior to the start of testing. The sensor holder has corresponding electrodes which are brought into
30 electrical contact with the conductive tracks of the test strip. Test devices are known in which a plurality of test strip are provided on a cartridge disc. Each strip is housed in its own sensor slot, and means are provided to eject a test strip from its slot when required, and to
35 automatically locate it in a sensor holder. Examples of

263654v1
19 July 2000

test devices with test strip dispensers are described in US Patent No. 5,660,791, European Patent Application No. 0 732 590, and European Patent Application No. 0 738 666.

5 A problem with test strips is that they have only a limited shelf life, and exposure of test strips to the atmosphere reduces the shelf life further. Test strips open to the atmosphere will typically have a shelf life of about two to three months, whereas test strips which are
10 sealed from the atmosphere will have a shelf life of about six to 12 months.

It has been proposed in WO 94/10558 to provide a stack of disposable test elements in a cylindrical housing, the
15 stack being urged towards a test station to form a liquid-proof seal. In DE 196 39 226 A1 it is proposed to provide a test device with a cartridge that may have a plurality of chambers containing test strips, each of which chambers may be individually sealed to preserve the shelf life of
20 the strips therein. A user removes the seal for each chamber when required, and a timing circuit may be activated either by the user or when the cartridge is pushed into the device. After a set time period has elapsed, an alarm or other indication reminds the user
25 that the time period for using the strips has elapsed.

It is an object of the present invention to provide an improved test device.

30 SUMMARY OF THE INVENTION

According to one aspect of the present invention there is provided a test device for testing of analyte concentration in a fluid to be applied thereto, the device
35 comprising:

2636a4v1
19 July 2000

- a) a plurality of test members arranged in at least one stack, each of said test members carrying reagent means for producing an electrical signal in response to the concentration of analyte in an applied fluid, each of said test members having a plurality of electrode tracks for transmitting said electrical signal;
- b) a housing having electrodes disposed therein for engaging with the electrode tracks on a test member at an engagement location;
- c) a meter connected to the said electrodes and disposed at least partly in the housing, having electronics means for producing a signal output which is dependent on the electrical signal from a test member when the test member is engaged with the said electrodes;
- d) a pusher which is adapted to push a single test member from the stack and into the engagement location where it can engage with the said electrodes and where the test member can be accessed to apply a fluid thereto;
- e) an actuation member operably connected to the pusher, the said actuation member being operable by a user to move the pusher;
- f) the or each stack of test members being enclosed in a magazine which is initially sealed by a moisture impermeable seal; and
- g) wherein means are provided for breaking the said seal and permitting a test member to be pushed from the magazine by the pusher when the first test member from the said magazine is to be used.
- The device may be disposable and may be pre-loaded with all the test members. At the point of final assembly, test member and meter calibration constants, expiry date information and units of measurement may be downloaded into the meter by suitable means, for example via a bi-directional RS232 bus. This has the advantage that each

2636a4v1
19 July 2000

meter may be uniquely matched to the specific batch of
test members used within the device. The meter and
associated test members can be quality controlled as a
single unit and by removing the need for a user to input
5 calibration data, as in a conventional meter, user error
of this function may be eliminated.

The software may also prevent the device from being used
outside the overall product expiry date and may be
10 programmed to prevent test members from an opened magazine
from being used beyond its specific expiry period.

Because the seal on a magazine is automatically broken
only when the first test member is to be used, the shelf
15 life of each stack is maximised, and the user is not
required to take any action other than to operate the
device.

The test members will typically be elongate test strips,
20 and the invention will be described herein with reference
to such test strips. However it will be understood that
the test members may be of any desired shape and profile.

In a preferred embodiment, a plurality of magazines are
25 provided in a movable cartridge. Each magazine is sealed
until a test strip therein is required for use, whereupon
the cartridge moves to bring the magazine into a position
for use, and the seal is broken. This process is
preferably automated and requires no user input. Any
30 number of magazines may be employed, each containing any
desired number of test strips. For example, each magazine
may have 20 test strips and there may be 5 magazines, so
that the device is usable for 100 readings before being
discarded.

35

2636a4v1
19 July 2000

The actuation member may be mechanically linked to the pusher, directly or indirectly, or it may be linked electronically, for example by actuating an electric motor which drives the pusher. In a preferred embodiment the
5 actuation member comprises a plunger which the user presses. The plunger may act on the pusher via another member, notably a sliding member which has a cam surface. It will be appreciated that many other suitable arrangements may also be employed.

10

The seal may be broken on one side by a blade past which the magazine is moved, to permit a test strip to be pushed out. The seal may be broken at the other side and along the top by one or more cutting surfaces at the leading
15 edge of the pusher, so that the pusher initially both cuts the seal and pushes the top test strip to the engagement location. However, it would also be possible for the pusher to cause the test strip to break through the seal without the need for a separate blade. To facilitate
20 this, the region of the seal through which the test strip will pass may be provided with a frangible line of weakness.

In a preferred embodiment, each test strip comprises a
25 base member having a working area to which the fluid is to be applied, containing the reagent means, and a non-working area adjacent to the working area, wherein the total thickness of the test member in at least a portion of the non-working area is at least as great as the total
30 thickness of the test member in the working area.

By making the non-working area at least as thick as the working area, scuffing or abrasion of the working area in a stack can be reduced. Moreover, if a compressive load
35 is applied to a stack of the test members, this may be

2636a4v1
19 July 2000

spread out over a greater area, thereby reducing the possibility of compressive damage to the working area.

5 In a preferred embodiment, at least a part of the non-working area is of greater total thickness than the thickness of the working area. This further reduces the likelihood of damage to the working area by scuffing or abrasion when in a stack. The difference in thickness is preferably from 1 to 20 μm , notably from 5 to 10 μm .

10

To build up the working area, a plurality of layers are sequentially applied to the base layer, for example by screen printing, typically with curing or drying steps between the application steps. The layers which are
15 printed typically comprise electrode patterns, a reagent layer, and a mesh layer (for spreading out an applied fluid). As a result of the application of these layers, the working area of a conventional electrochemical test strip is typically about 100 μm thicker than the non-
20 working area, which contains the electrode tracks and, typically, a dielectric layer. A stack of 100 test strips will therefore be about 10 mm thicker in the working area than in the non-working area. In a test strip in accordance with the present invention, at least a part of
25 the non-working area may be made thicker by any suitable means. Suitable means include, for example: a printed relief ink; an applied pad or tape; embossing of the base layer or an intermediate layer; or an extension of the mesh layer from the working area.

30

Further objects and advantages of the invention will be apparent as the description proceeds.

2636a4v1
19 July 2000

BRIEF DESCRIPTION OF THE DRAWINGS

The invention will now be further described by way of example with reference to the following drawings, in which:

- Figure 1 illustrates user actions in operating a test device in accordance with the present invention;
- 10 Figure 2 shows the assembly of a cartridge for use in the device of Figure 1;
- Figure 3 illustrates the action of the pusher in opening the seal on a magazine;
- 15 Figure 4 illustrates the action of the pusher on a test strip;
- Figure 5 shows a mechanism for operating the pusher;
- 20 Figure 6 is an exploded view of part of the device of Figure 1;
- Figure 7 is an exploded schematic view illustrating the cartridge advance mechanism;
- 25 Figure 8 shows steps in the advance of a cartridge;
- Figure 9 shows sectional views through part of the cartridge advance mechanism at different stages;
- 30 Figure 10 illustrates an alternative embodiment in which magazines are releasably connected together; and

35

2636a4v1
19 July 2000

Figure 11 is a top plan view of a test strip in a preferred embodiment of the invention.

DETAILED DESCRIPTION

5

The test device shown in Figure 1 comprises a housing 2 which houses a meter with a visible display 4, in this example, an LCD. A plunger 6 is released for use by the user pressing a release button which operates a catch.

10 Figure 1a shows the device after a user has depressed the release button with his right index finger. To take a reading of blood glucose concentration, the user partially depresses the plunger 6 to an intermediate position, causing a test strip to be presented for receiving a
15 sample of blood (Figure 1b). After the blood has been applied to the test strip, a reading is displayed on the display 4 (Figure 1c). The user then fully depresses the plunger 6 so that it is again engaged by the catch, causing the test strip to be ejected. The device is then
20 ready for another reading to be taken. Figure 1d illustrates the device after the test strip has been ejected and after the user has again pressed the release button to free the plunger 6. The various mechanisms involved in this process will be described below.

25

As shown in Figure 2, a stack of test strips 8 is loaded in a magazine 10, which is in turn located in cavity 74 in a cartridge 12. In this example there are five cavities 74, each of which houses spring means 14, in this example
30 a helical spring. Each cavity has an opening 18 through which a test strip 8 will be pushed by a pusher 16. The spring urges the stack of test strips 8 upwards so that the top strip is engageable by the pusher 16. A foil seal
20 seals the cavities 74 containing the magazines 10. The
35 slitting of the foil seal 20 will be described below, with

2636a4v1
19 July 2000

reference to Figure 3, which shows progressive movement of the pusher 16.

Advancement of the cartridge 12 moves it past a blade 22 which is mounted in the housing 2 of the test device. The blade 22 makes a slit in the foil seal 20 at one end, through which a test strip 8 is to be pushed. The pusher 16 is moved from one end of the cavity 74 to the other, as illustrated by positions (1) through (5) of Figure 3. As the pusher 16 moves, cutting surfaces 24 on its leading edge cut the foil seal 20 and push the uppermost test strip 8 out through the opening 18 to the testing position (4) (corresponding to that shown in Figure 1b), where a test reading can be taken. Fully depressing the plunger 6 moves the pusher 16 further towards the opening 18 and ejects the test strip 8. In subsequent drawings, the seal 20 is omitted for clarity.

Referring now to Figure 4, a mechanism is illustrated whereby movement of the pusher 16 from the position in Figure 4a initially pushes the test strip 8 out of the housing and then the head 28 of the pusher 16 bears down on the electrodes 26 of the meter so as to bring them into engagement with electrode tracks on the test strip 8 (Figure 4b). After a reading has been taken, further advance of the pusher 16 (Figure 4c) takes the head 28 beyond the electrodes 26, which disengage from the test strip 8 and permit the pusher 16 to eject the test strip.

The mechanism for advancing the pusher 16 is illustrated in Figure 5. The assembly shown in Figure 5 comprises a slider 32 which is operatively connected to the plunger 6. The slider 32 is slidably mounted on a chassis top 36 which receives a groove plate 34. The groove plate 34 has a groove therein which receives a sprung detent member 52

2636A4v1
19 July 2000

of the slider 32, the function of which will be described later. Also provided on the slider 32 is a ratchet driver 44 which engages with a ratchet wheel 40, the operation of which will be described later. A ratchet driver guide 38 is provided on the housing base 42. The back housing member 46 (and front housing member 64 - Figure 6) have cartridge tracks therein, along which the cartridge 12 can move. In the start position shown in Figure 5a, the user presses the release button (not shown) where indicated by the arrow 30. This releases a catch 58 (Figure 6) on the slider 32. A spring 60 (Figure 6) pushes the plunger 6 and the slider 32 in the direction of the large arrow in Figure 5b. The slider 32 has a hockey stick-shaped slot 31 in which is received the pusher 16. As the slider 32 travels, it moves the pusher 16 in the direction of the small arrow 50 shown in Figure 5b. At 6 mm before the end of travel, the pusher 16 is removed from the cartridge 12. In the final 6 mm of travel the ratchet driver 44 indexes the ratchet wheel by one position, and advances the cartridge 12 so that the foil 20 on the first magazine 10 is slit at one end. The user then pushes the slider 32 to an intermediate position (Figure 5c) and in so doing, causes the pusher 16 to move back, with its cutting surfaces cutting the foil as previously described, and pushing the uppermost test strip out of the housing 2. The slider 32 is held in the intermediate position by engagement of the sprung detent member 52 in the groove of the groove plate 34. The detent member 52 and groove plate 34 operate in the manner of a ballpoint pen advancing and retracting mechanism, with the detent member 52 cycling around the groove in the course of one test cycle. After a reading has been taken, the plunger 6 is then fully pushed in by the user (Figure 5d), causing the slider to return to the position shown in Figure 5a and causing the pusher to eject the used test strip 8. The

2636a4v1
19 July 2000

slider 32 is now held in place until the next test reading is required. Figure 6 shows some of the components more clearly, including the chassis cartridge end 70 which has a cartridge drive spring 68. A pusher "parking slot" plug 56 is mounted in the back housing member 46, where the pusher 16 is kept away from the cartridge 12 to permit movement of the cartridge. An optional sensor exit slot plug 66 is provided in the front housing member 64. A PCB 54 provides the meter electronics. When the test device is first used, and when a magazine is first opened up, a microprocessor on the PCB starts a timer counting down whereby the display 4 indicates when a particular magazine has exceeded its recommended life, or in the event that all magazines have exceeded their shelf life.

Figure 7 shows the cartridge advance mechanism as an exploded schematic, with the cartridge in half-section. The cartridge 12 is urged by the spring 68 in the direction of the arrow 72. Underneath the cartridge 12 there is provided a plurality of cartridge location pegs 76, which are spaced apart by the width of the magazines, ie the distance between the centre lines of the magazines 10. There is a peg 76 for each cavity 74, and an additional leading peg on a front lip of the cartridge 12. The ratchet wheel 40 has a keyway 78 thereon for the cartridge location pegs 76 to pass through as the cartridge 12 advances. The ratchet wheel is driven by the ratchet driver 44 which, cooperating with a pawl 62, drives the ratchet wheel 40 in a clockwise direction as viewed in Figure 7. The ratchet driver 44 reciprocates in both directions (80), but is sprung only in the direction indicated by the arrow 82. A cartridge final stop member 84 is provided at the proximal end of the housing base 42.

2636a4v1
19 July 2000

After each advance of the cartridge 12, it remains stationary until the test strips in a magazine have been used up. At this point the cartridge 12 advances by the width of a magazine. The mechanism for controlling advance of the cartridge 12 is described with reference to Figures 8 and 9. Starting from the position shown in Figure 8a, the ratchet mechanism is in a rest position ready for use. The centre line 86 of the active magazine 12 is in the keyway of the ratchet wheel 40. The user presses the release button and the ratchet driver 44 travels in the sprung direction (arrowed - Figure 8b). The ratchet driver 44 engages the ratchet wheel (Figure 8c) and rotates or indexes the ratchet wheel by one place (arrowed - Figure 8d). Figures 8d through 8h shows the cartridge advancement sequence. As the ratchet wheel 40 advances from the position shown in Figure 8e to that of Figure 8f, the two foremost location pegs 76 of cartridge 12 are freed to advance through the keyway 78. The location peg 76 furthest to the left in Figure 8f acts against the inclined surface of the keyway 78 while exiting the keyway. This forces the ratchet wheel 40 to rotate one place (Figure 8g) while the second location peg 76 is moved to the centre of the ratchet wheel. The rotation of the ratchet wheel 40 presents a solid stop wall at the point 88 to the oncoming location peg. At the position shown in Figure 8h, the cartridge has advanced by one magazine width, and the location peg 76 of the magazine behind the new active magazine comes to rest against the ratchet wheel stop wall, aligning the next magazine ready for use.

When the cartridge 12 is loaded in the housing during manufacture, the front location peg 76 is located in the keyway 78 and the ratchet wheel 40 is located so that the first time the ratchet wheel is indexed, the foremost

2636a4v1
19 July 2000

magazine 10 is advanced as describe above, and the seal is cut by the blade 22.

Because there are 20 test strips per magazine, and 20
5 teeth on the ratchet wheel, the ratchet wheel is constructed to permit cartridge advance only once during a complete (360°) rotation. Figures 8i and 9a show how, with the ratchet wheel at position 10 (180° rotation), the cartridge 12 is prevented from premature advancement. The
10 cartridge location peg 76 is prevented from entering the ratchet wheel keyway 78 through incorrect orientation and misalignment. The cartridge base 90 and location peg 76 are shown separated from the ratchet wheel in Figures 9a and 9b for clarity. With the ratchet wheel at position 11
15 (Figures 8j and 9b) the location peg 76 is also misaligned with the ratchet keyway 78 and the cartridge does not advance.

An alternative embodiment is illustrated with respect to
20 Figure 10. Here, the magazines are releasably connected together, in this example by a dovetail joint (Figure 10b). Used magazines 10 project through an opening in the housing and can be removed by the user. Figure 10a shows plan views before (top) and after (bottom) a used magazine
25 has been slid off from its neighbour. In this embodiment the housing can be made smaller because it need not accommodate used magazines.

The test strip 8 shown in Figure 11 comprises a planar
30 base member 92, in this example of poly(butylene terephthalate) (PBT) (Valox® FR-1 from GE Plastics). The strip is 30 mm x 5.5 mm, and 0.5 mm thick. A working area 94 is of conventional construction, comprising a plurality of electrodes, a reagent layer in intimate contact with

2636a4v1
19 July 2000

the electrodes, and a mesh layer for spreading out a drop of fluid to be received on the working area. Electrode tracks 102, for example of carbon, in the non-working area 98 of the test strip are connected to the electrodes in the working area 94 in known manner. Also in known manner, a dielectric layer 96 is printed around the working area 94 so as to overlies a portion of the electrode tracks 102, leaving just the ends of the tracks exposed for connection to corresponding 26 electrodes on the meter. The layers are applied to the base member as inks, by screen printing. Each ink layer is about 10 to 20 μm thick, and the mesh is about 59 to 67 μm thick. The working area 94 has a total thickness which is about 100 μm thicker than the non-working area 98 up to the dielectric layer 96.

To increase the thickness of parts of the non-working area, a high relief ink 100 has been printed in four strips. The high relief ink has a dried thickness such that the total thickness of the non-working area to which the high relief ink 100 has been applied is slightly greater than the total thickness of the test strip in the working area 94. Thus, when a stack of such test strips 8 is formed, and a compressive load is applied to the stack by the spring 14, the working area 94 will not bear all the compressive load. Scuffing of the test area will be reduced compared to a conventional test strip in which the working area stands proud of the non-working area.

Although this embodiment has been illustrated with reference to the use of a high relief ink printed in strips, it will be understood that it is not limited to this embodiment. The ink could be printed as a continuous block, and it could entirely surround the working area if desired. Instead of, or in addition to, the high relief

2636a4v1
19 July 2000

ink, other means could also be provided to increase the thickness of the non-working area, for example: an applied pad or tape; embossing of the base layer or an intermediate layer; or an extension of the mesh layer from
5 the working area into the non-working area.

Although the invention has been described with reference to a test device for measuring blood glucose concentration, it is to be understood that the invention
10 is not limited to this application. The invention may be used in the determination of any analyte in a fluid by the use of suitable reagents in the test strip. Such reagents are well known to those skilled in the art.

2636a4v1
19 July 2000

CLAIMS

1. A test device for testing of analyte concentration in a fluid to be applied thereto, the device comprising:
- 5 a) a plurality of test members arranged in at least one stack, each of said test members carrying reagent means for producing an electrical signal in response to the concentration of analyte in an applied fluid, each of said test members having a plurality of electrode tracks for
10 transmitting said electrical signal;
 - b) a housing having electrodes disposed therein for engaging with the electrode tracks on a test member at an engagement location;
 - c) a meter connected to the said electrodes and disposed
15 at least partly in the housing, having electronics means for producing a signal output which is dependent on the electrical signal from a test member when the test member is engaged with the said electrodes;
 - d) a pusher which is adapted to push a single test
20 member from the stack and into the engagement location where it can engage with the said electrodes and where the test member can be accessed to apply a fluid thereto;
 - e) an actuation member operably connected to the pusher, the said actuation member being operable by a user
25 to move the pusher;
 - f) the or each stack of test members being enclosed in a magazine which is initially sealed by a moisture impermeable seal; and
 - g) wherein means are provided for breaking the said seal
30 and permitting a test member to be pushed from the magazine by the pusher when the first test member from the said magazine is to be used.

2. A device as claimed in claim 1, wherein the test
35 members are arranged in a plurality of stacks, each one

2636a4v1
19 July 2000

enclosed in a magazine which is initially sealed by a moisture impermeable seal, the magazines being movable so as to enable each in turn to reach a position in which the pusher can break the seal and push a test member therefrom.

3. A device as claimed in claim 1 or claim 2, wherein operation of the actuation member causes the pusher to engage with the electrodes and bring them into contact with the electrode tracks on the test member when the test member is in the engagement location.

4. A device as claimed in any one of the preceding claims, wherein further operation of the actuation member causes the pusher to push a test member from the engagement location and eject the test member from the housing.

5. A device as claimed in any one of the preceding claims, wherein blade means are provided in the housing for cutting the seal to form a slit through which a test member can pass when pushed by the pusher.

6. A device as claimed in claim 5, wherein the blade is fixed, and the magazine is movable so that the slit will be cut when the magazine moves.

7. A device as claimed in claim 1 wherein the pusher is provided with at least one cutting surface for cutting the foil seal.

8. A device as claimed in claim 7, wherein the foil seal is provided with a frangible line of weakness at a location where a test member is to pass through, whereby when a test strip is urged against the said line of

2636a4v1
19 July 2000

weakness by the pusher, the foil will break and permit passage of the test member.

9. A device as claimed in claim 2, wherein the cartridge
5 is urged by spring means towards a ratchet wheel which has
a keyway therein, the cartridge being provided with a
plurality of spaced apart location pegs for locating in
the keyway and the ratchet wheel only permitting entry of
a location peg when the ratchet wheel is in a defined
10 orientation.

10. A device as claimed in claim 9, wherein operation of
the actuating member causes indexing of the ratchet wheel.

11. A device as claimed in any one of the preceding
15 claims, further comprising a sliding member which has an
angled slot therein which provides a cam surface that
bears against the pusher, whereby movement of the sliding
member in a first direction causes movement of the pusher
20 in a second direction.

12. A device as claimed in any one of the preceding
claims, further comprising spring means which urge the
stack of test members towards the seal.
25

13. A device as claimed in any one of the preceding
claims, further comprising means for releasably detaining
the pusher when the test member is in the engagement
location.
30

14. A device as claimed in any one of the preceding
claims, further comprising a processor and means for
initiating a timer at a predetermined time or when a
magazine is first opened, the processor being programmed
35 to provide a visible warning or message if a magazine

2636a4v1
19 July 2000

which is in use exceeds its shelf life or if unopened magazines exceed their shelf life.

15. A test device as claimed in any one of the preceding
5 claims, wherein the analyte to be tested for is glucose
and the fluid to be applied is blood.
16. A test device as claimed in claim 2, wherein the
10 magazines are releasably connected together and wherein
the housing has an opening through which used magazines
will project.
18. A test device as claimed in any one of the preceding
15 claims, wherein each test member in the or each stack
comprises a base member having a working area to which the
fluid is to be applied, containing the reagent means, and
a non-working area adjacent to the working area, wherein
the total thickness of the test member in at least a
20 portion of the non-working area is at least as great as
the total thickness of the test member in the working
area.
19. A test device as claimed in claim 18, wherein the
25 total thickness of the test member in at least a part of
the non-working area is greater than the total thickness
of the test member in the working area.
20. A test device for testing of analyte concentration in
30 a fluid to be applied thereto substantially as herein
described with reference to or as shown in the drawings.

262624v1
19 July 2000

ABSTRACT

TEST DEVICE

5 A test device for testing of analyte concentration in a fluid to be applied thereto, the device comprising a plurality of test members (8) arranged in at least one stack and electrodes (26) for engaging with electrode tracks on a test member (8). A pusher (16) pushes a
10 single test member from the stack so that it can engage with the electrodes. An actuation member (6) is operably connected to the pusher (16), and moves it when operated by a user. The or each stack of test members is enclosed in a magazine (10) which is initially sealed by a moisture
15 impermeable seal (20), and means (22, 24) are provided for breaking the seal (20) and permitting a test member (8) to be pushed from the magazine (10) by the pusher (16) when the first test member (8) from the magazine (10) is to be used.

20

Figure 6

2636a4v1
19 July 2000

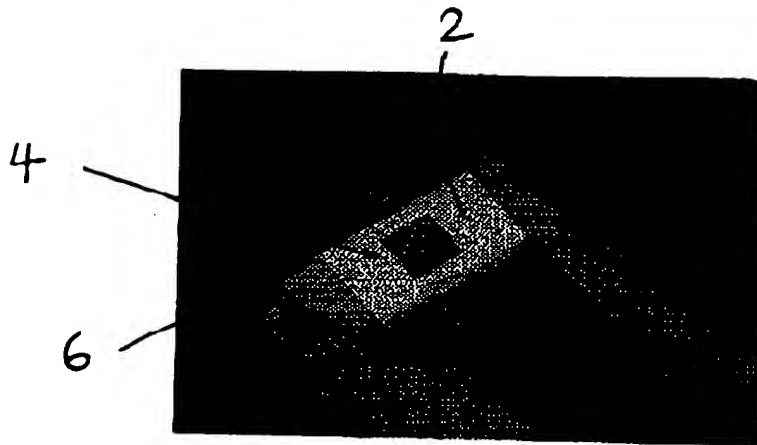


FIG. 1a

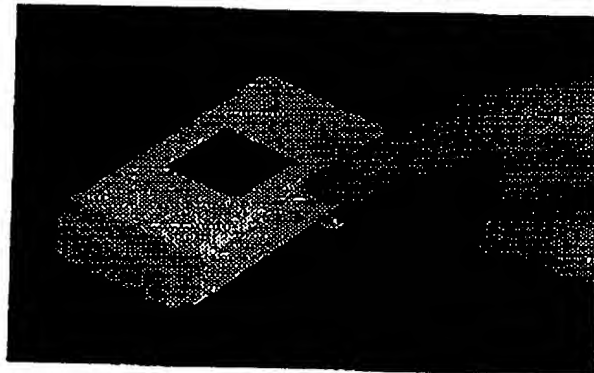


FIG. 1b

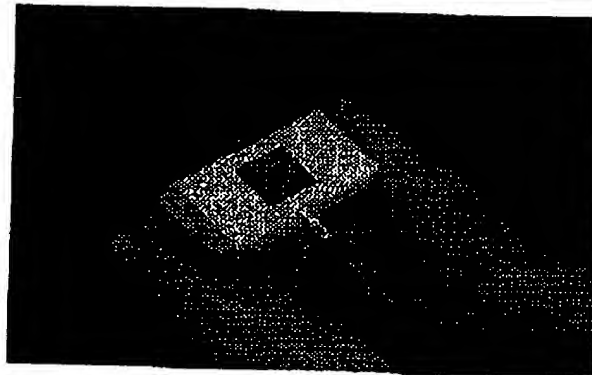


FIG. 1c

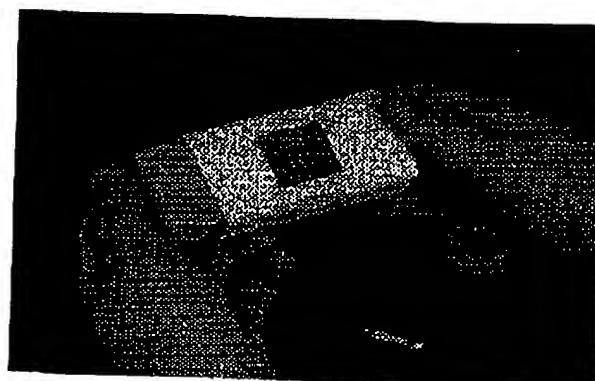


FIG. 1d

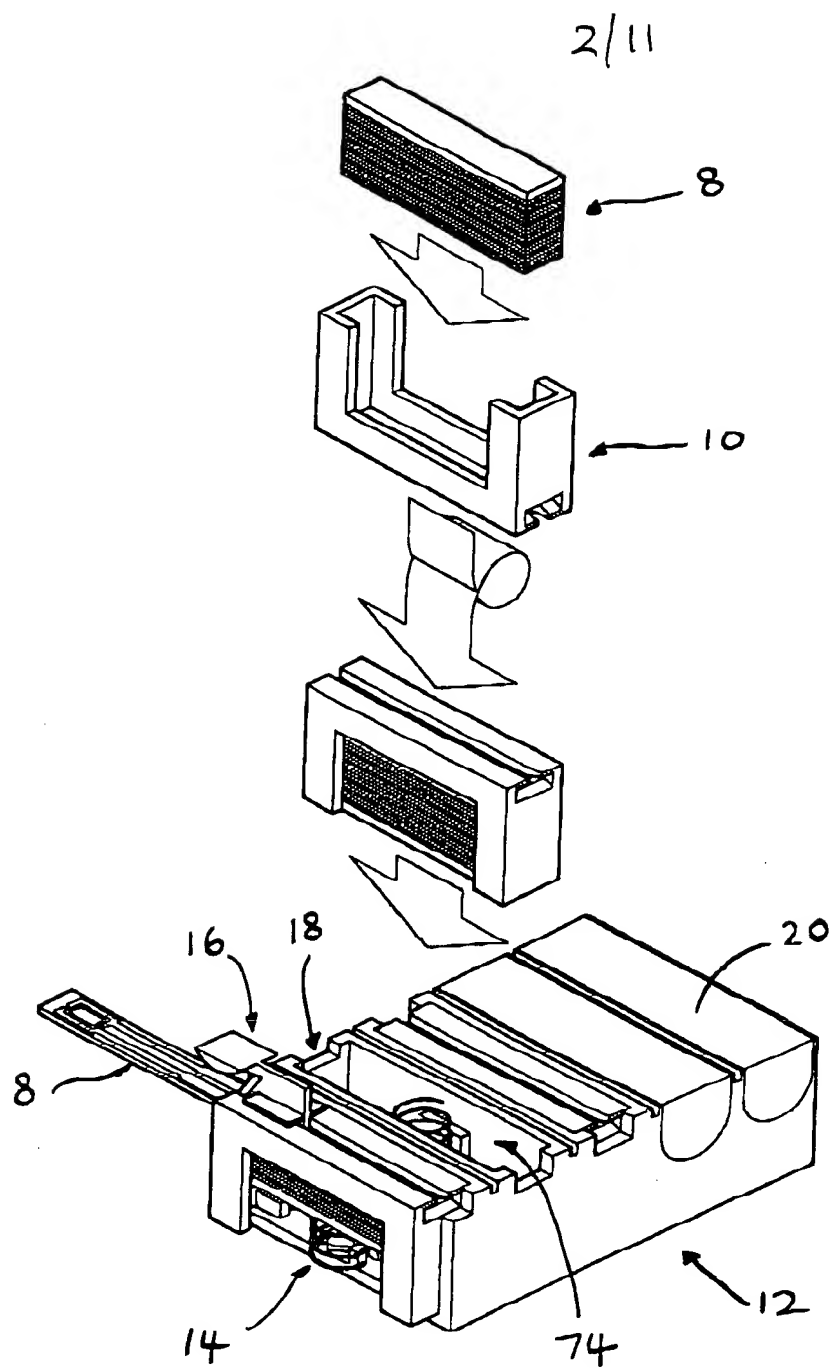


FIG. 2



3/11

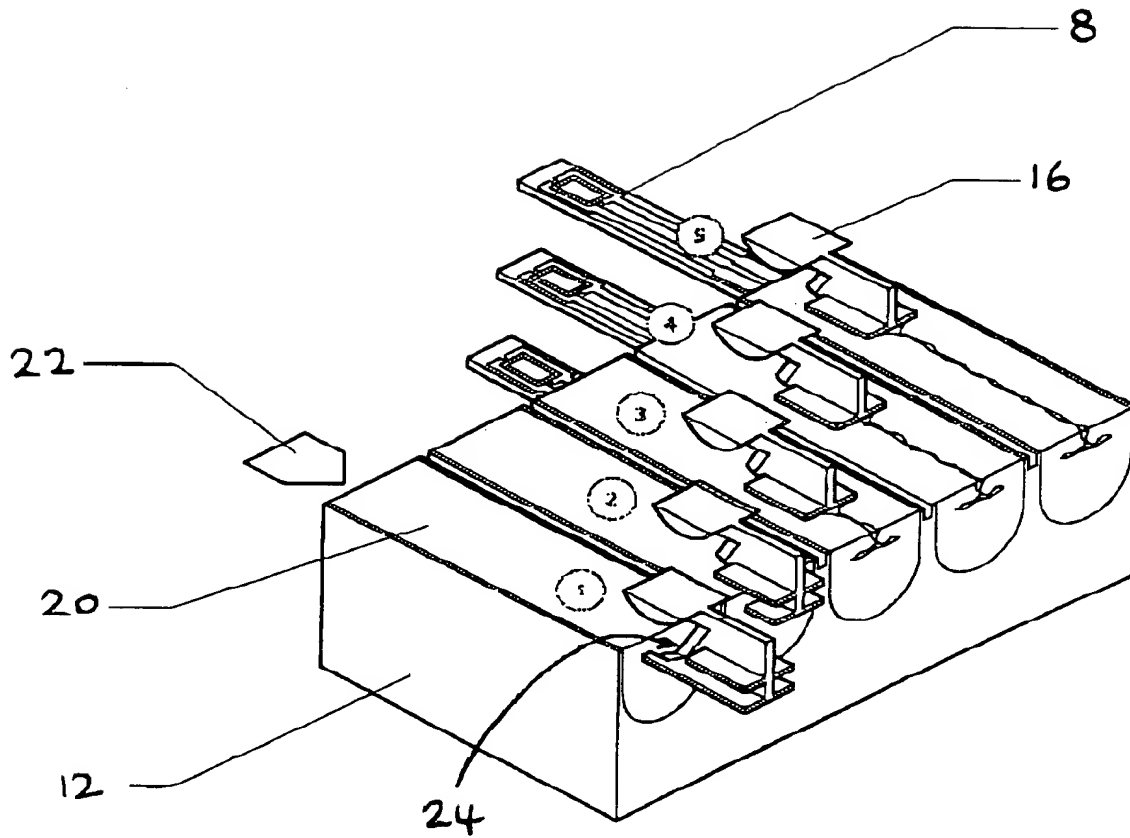


FIG. 3

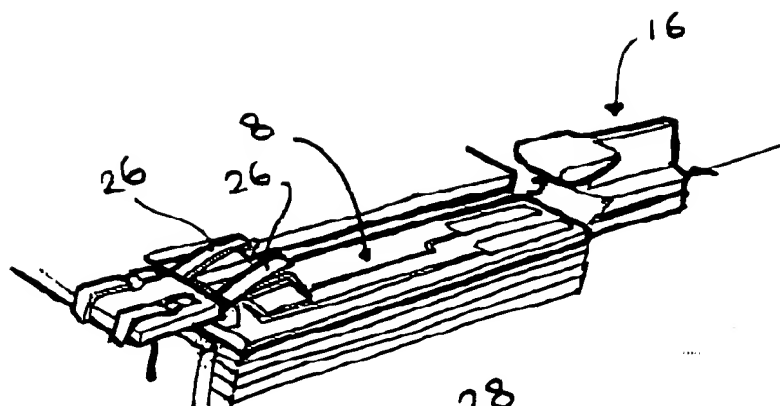


FIG. 4a

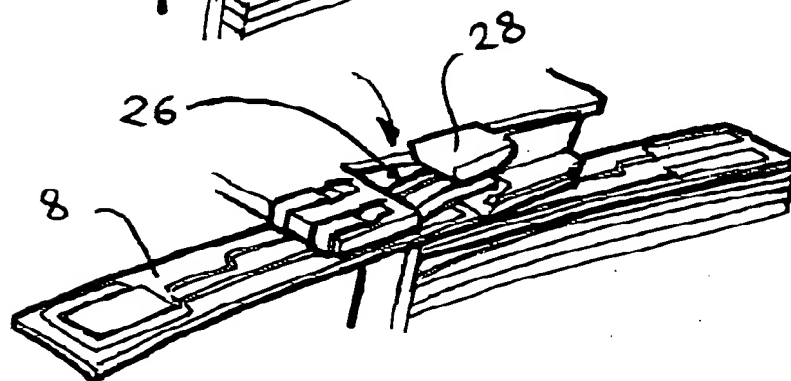


FIG. 4b

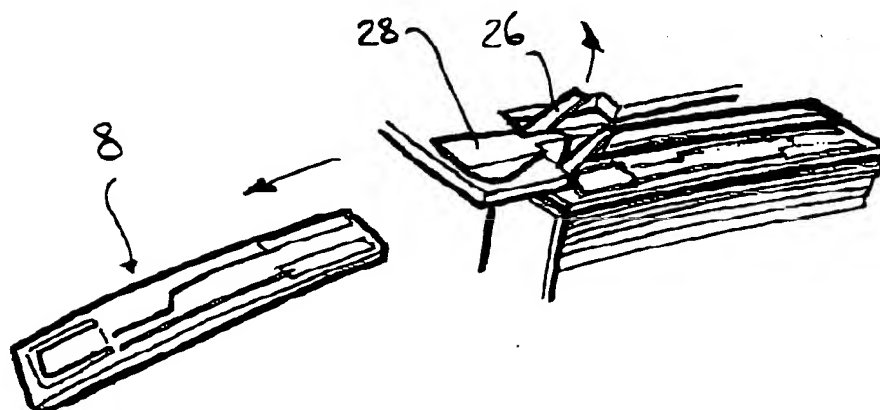


FIG. 4c

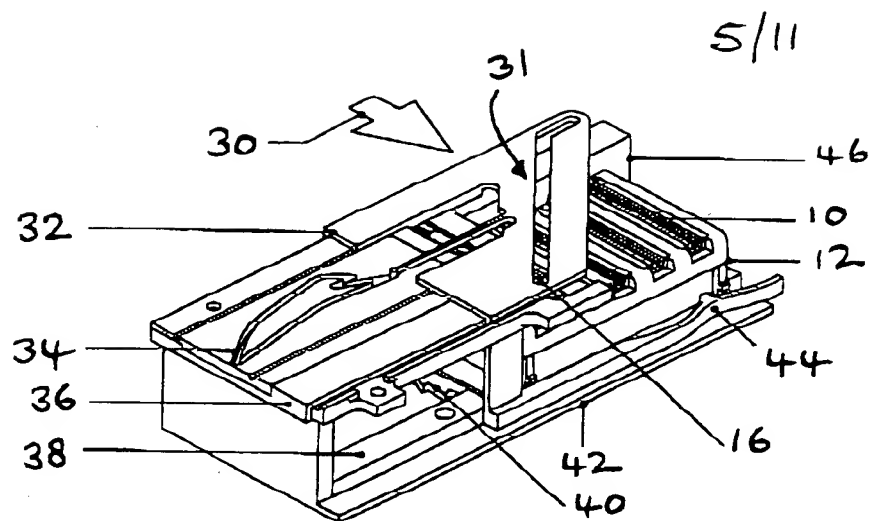


FIG. 5a

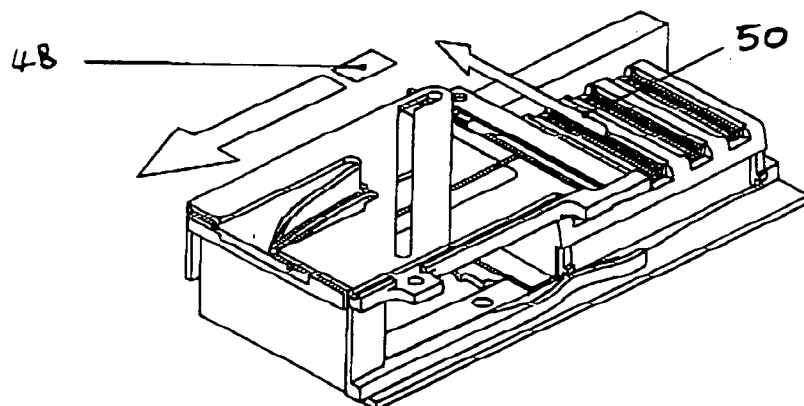


FIG. 5b

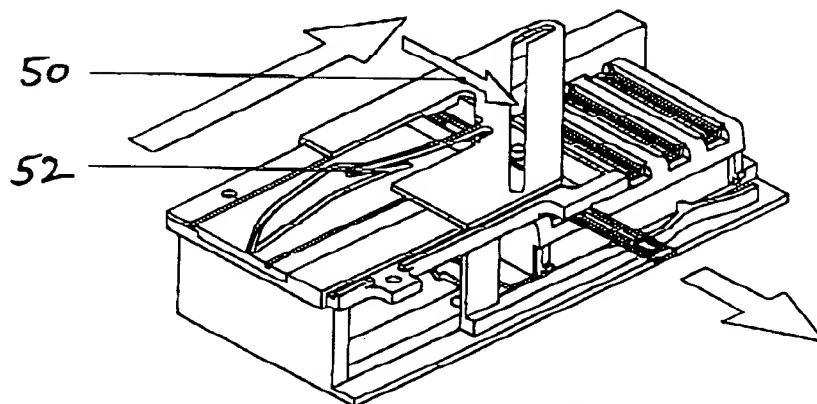


FIG. 5c

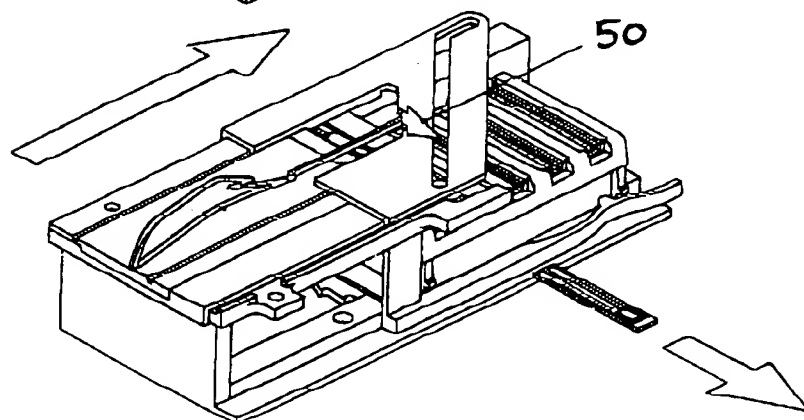


FIG. 5d

6/11

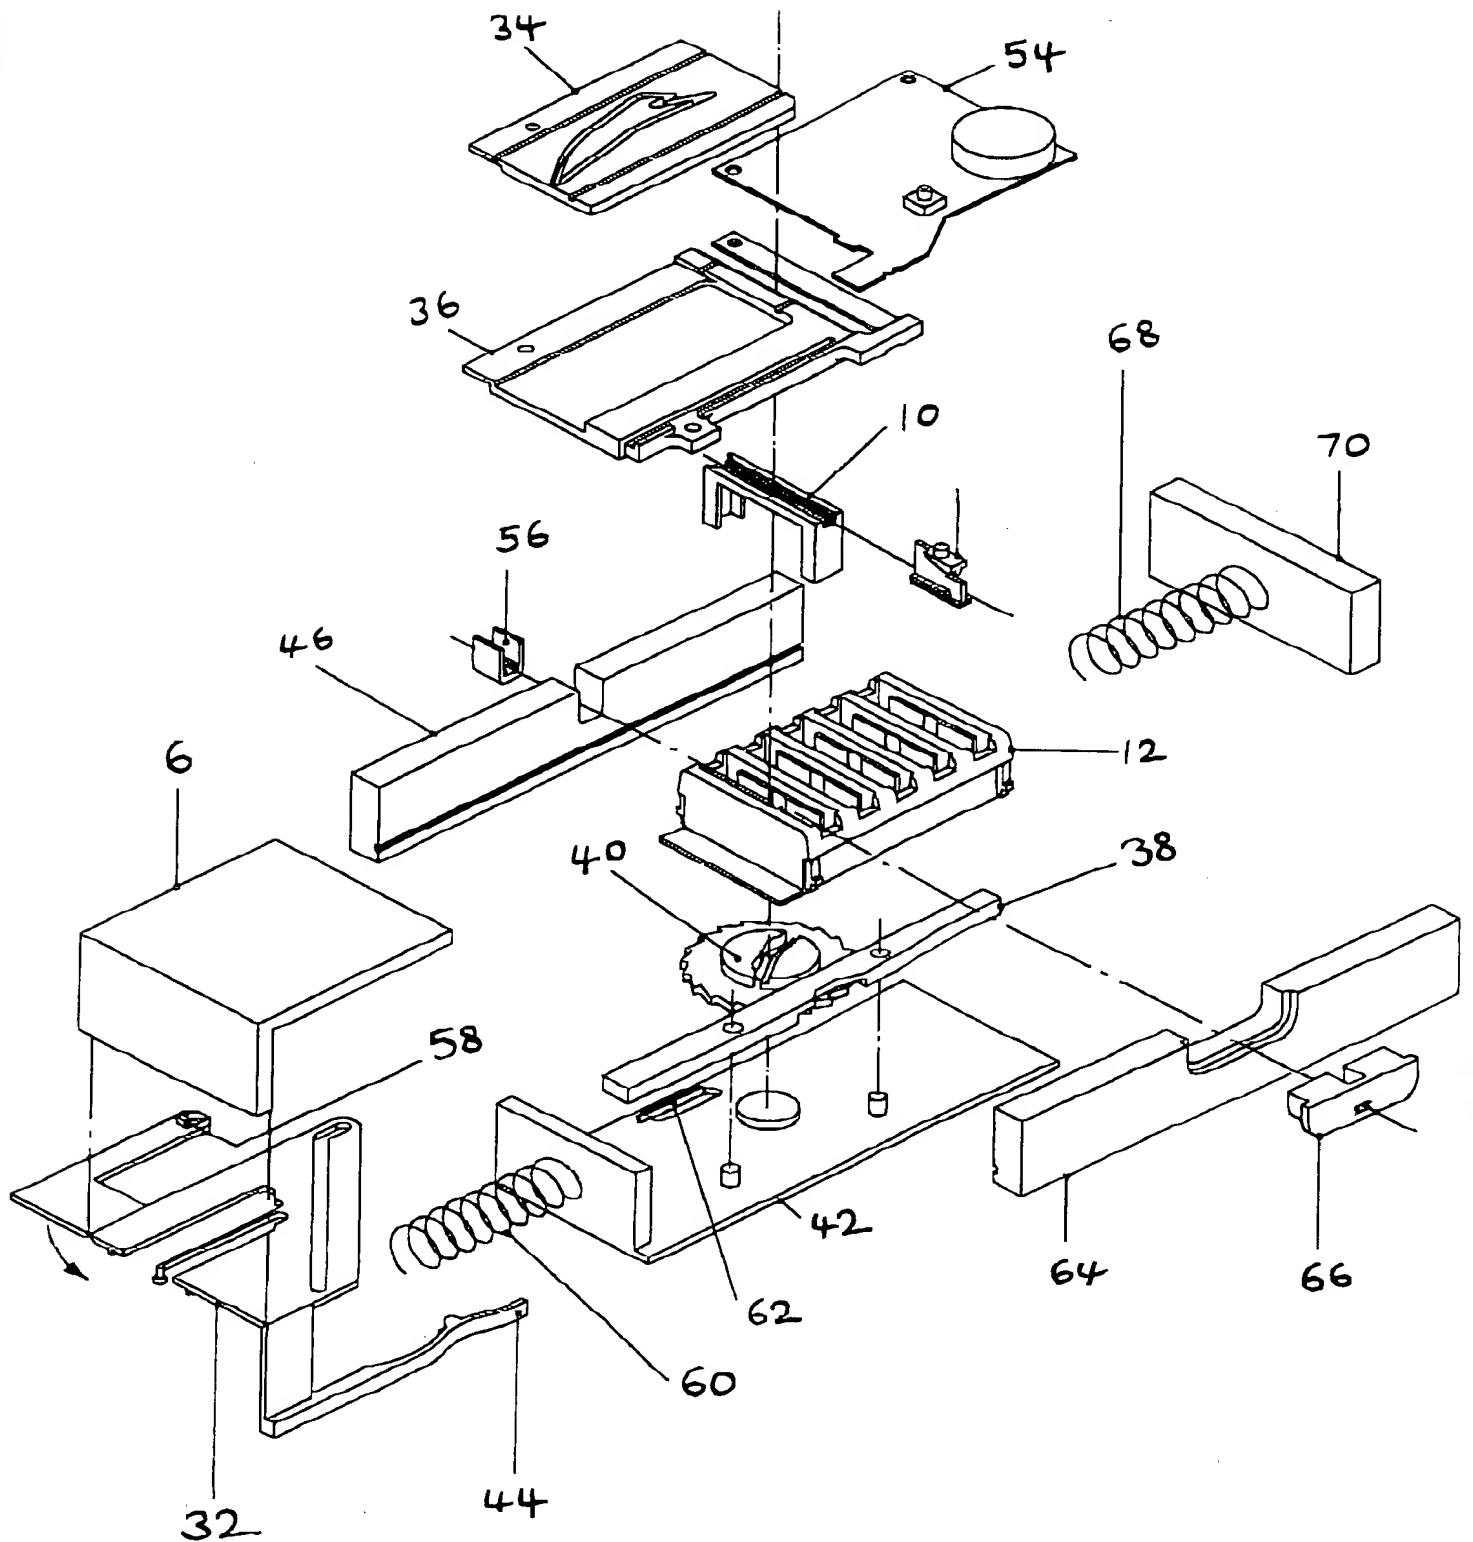


FIG. 6

7/11

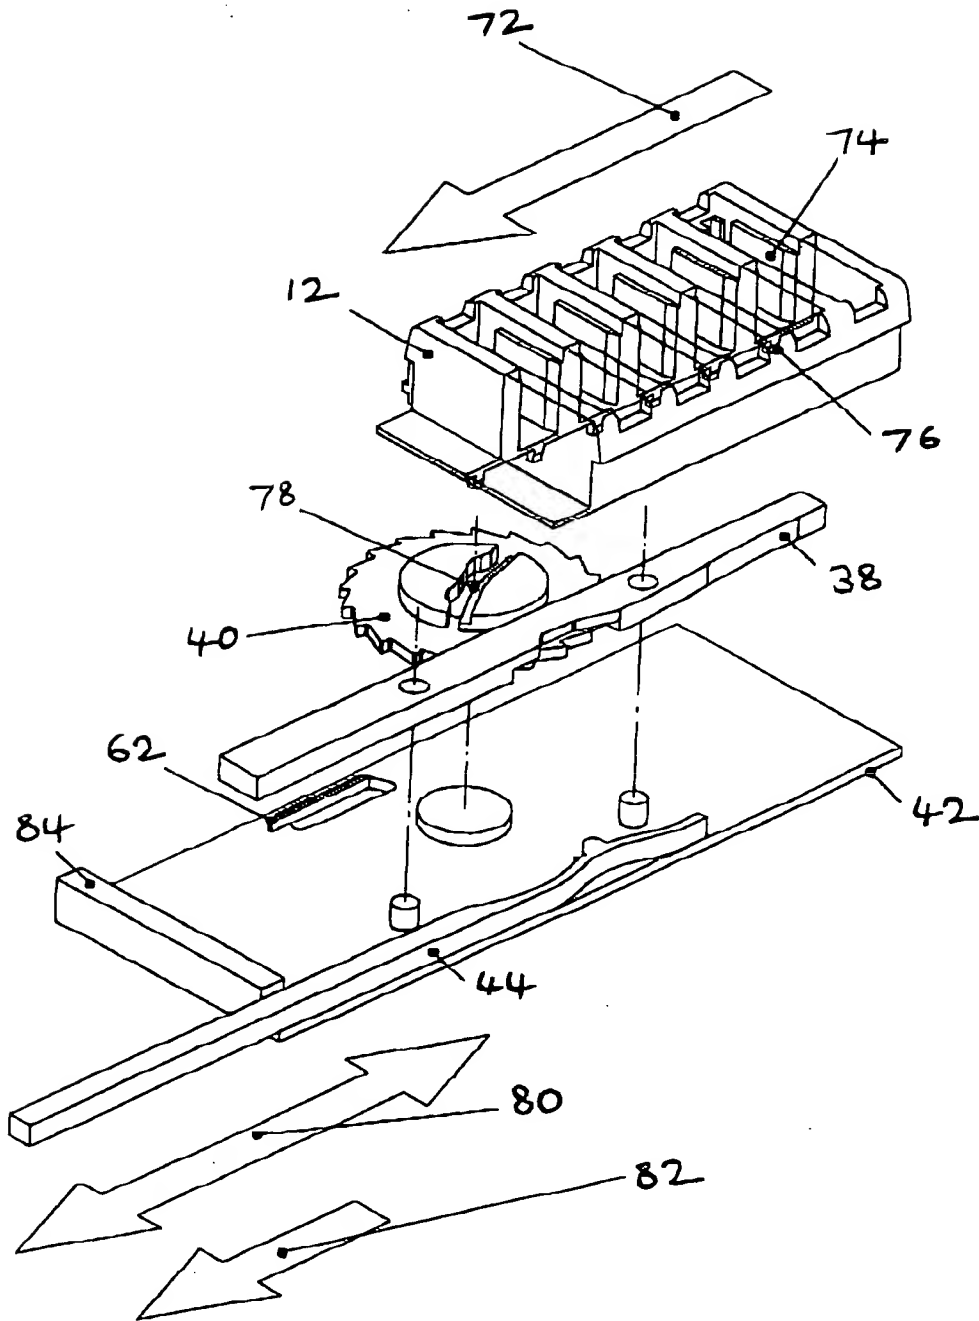


FIG. 7

8/11

FIG. 8a

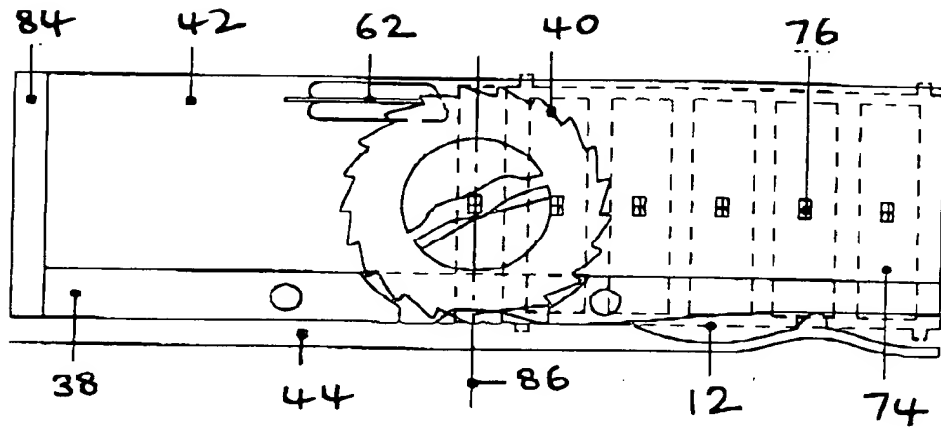


FIG. 8b

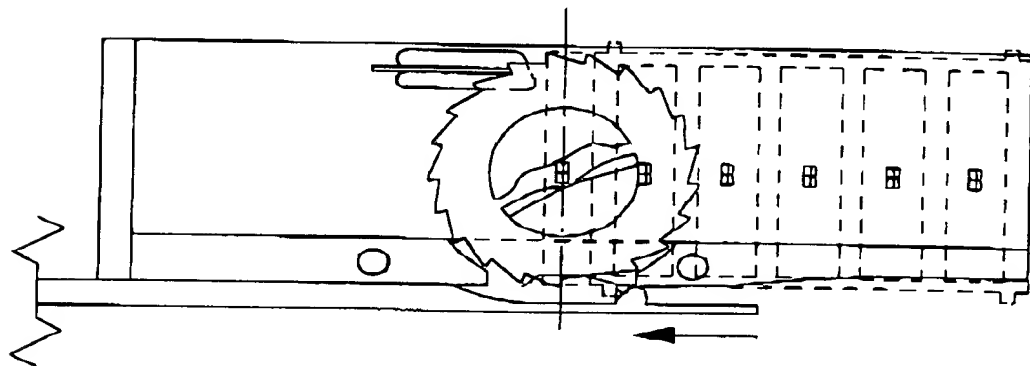


FIG. 8c


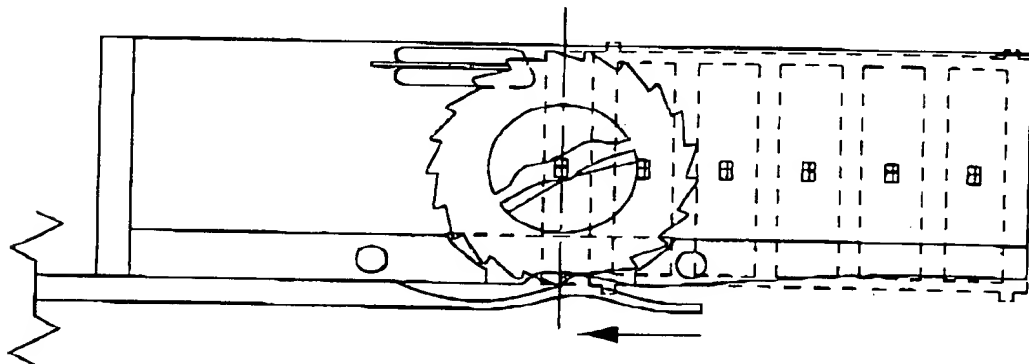


FIG. 8d



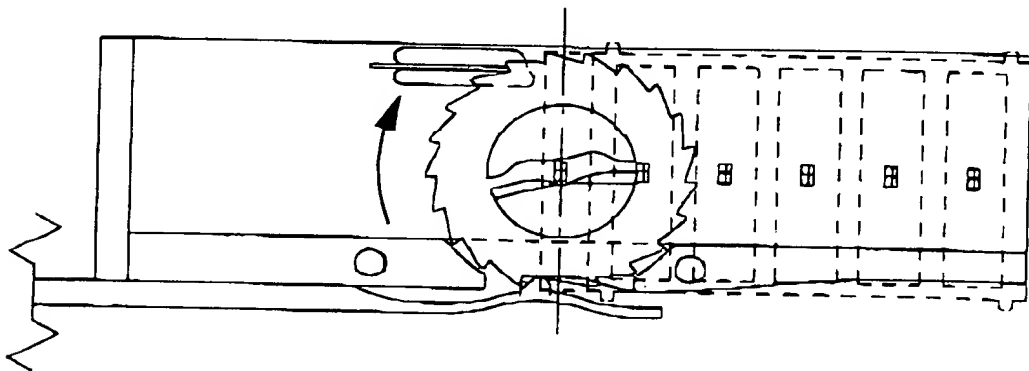

9/11

FIG. 8e

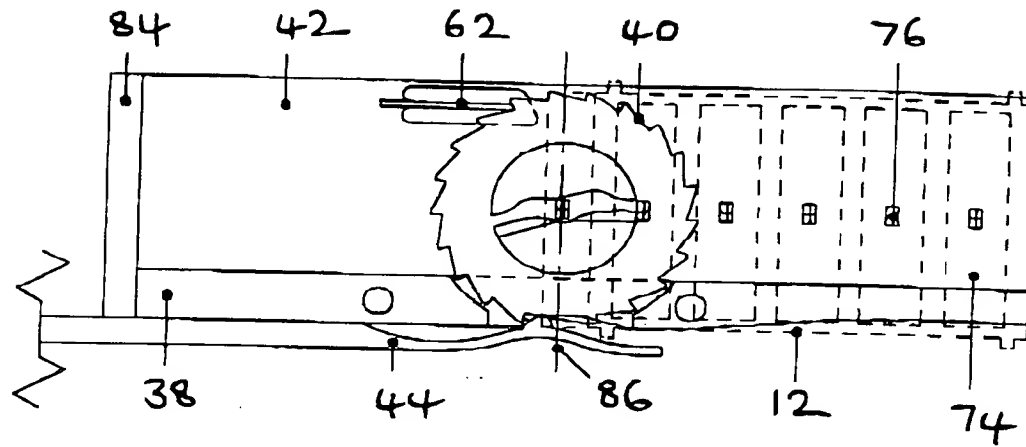


FIG. 8f

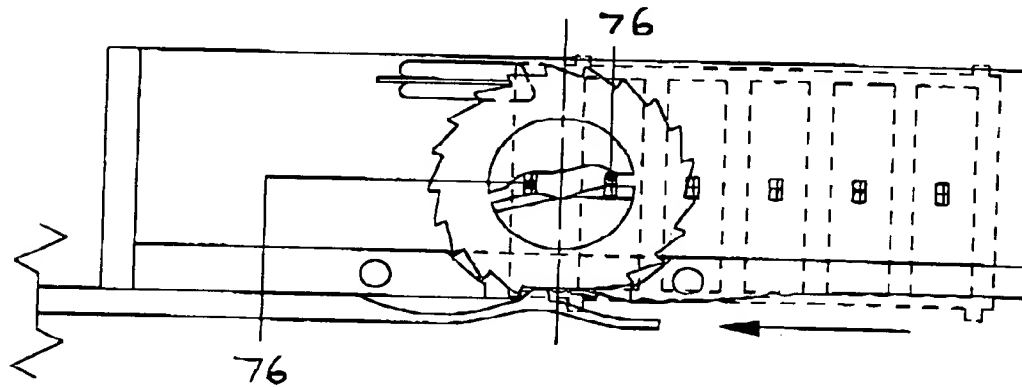


FIG. 8g

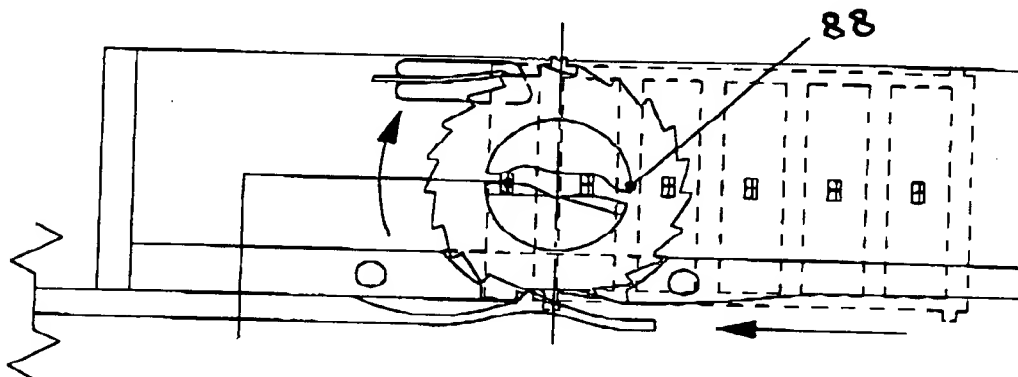


FIG. 8h

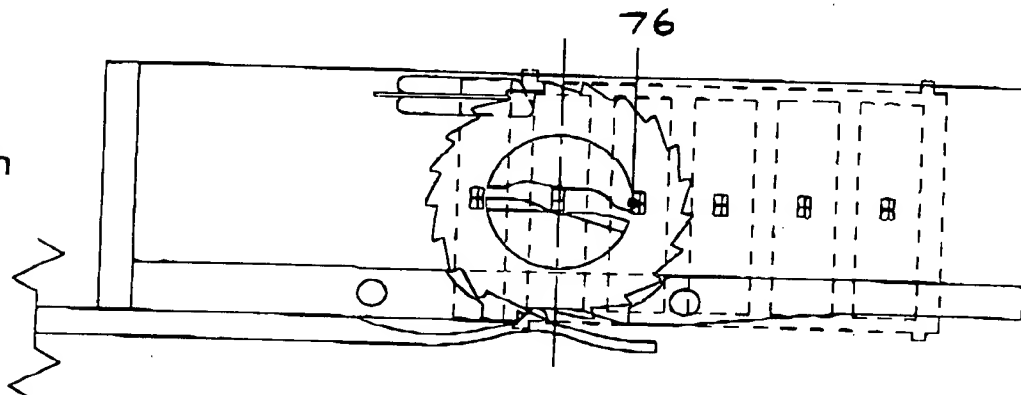


FIG. 8i




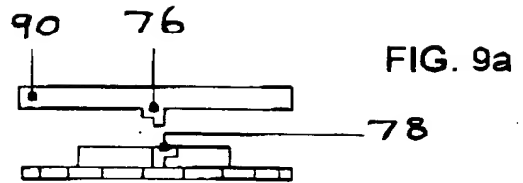


FIG. 8j

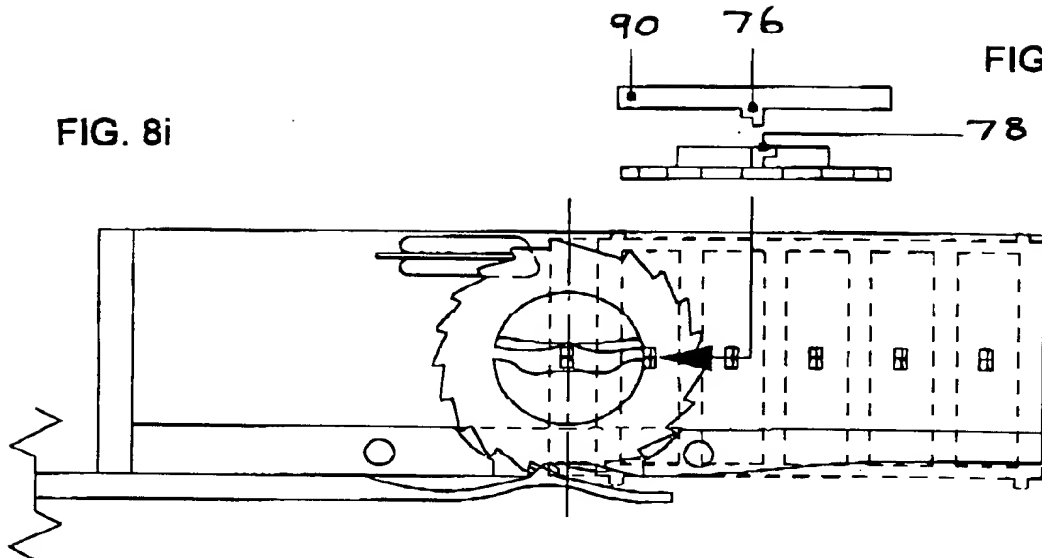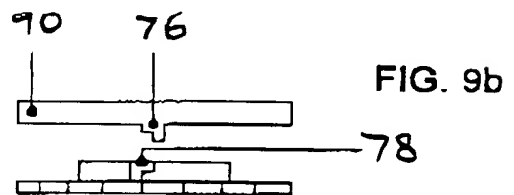

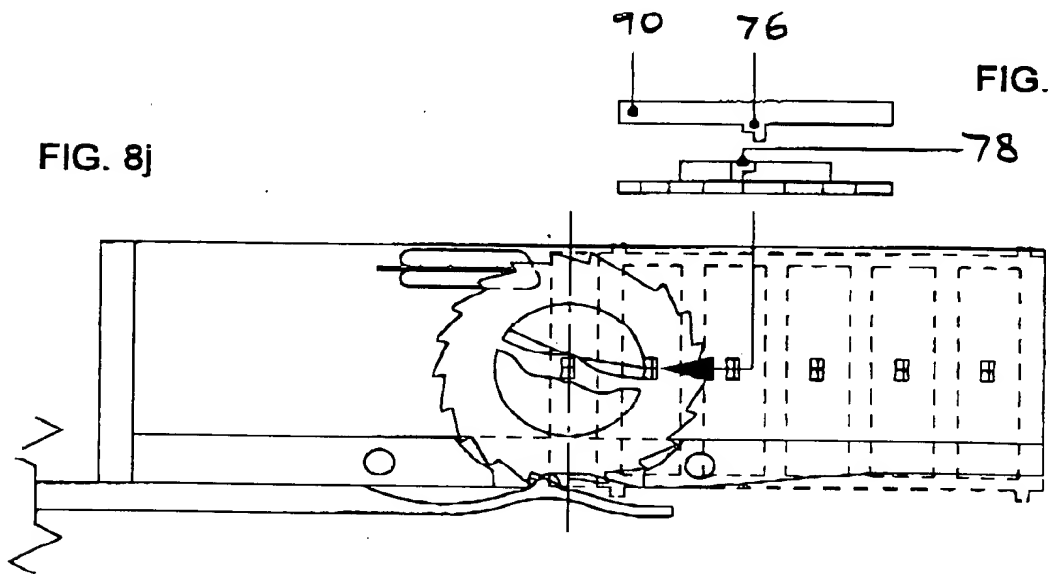

11/11

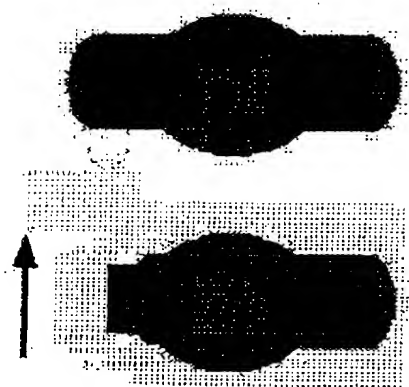


FIG. 10a

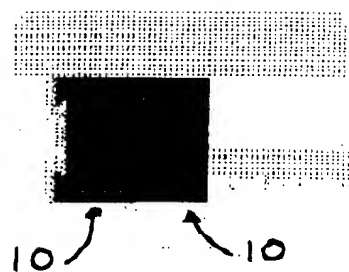


FIG. 10b

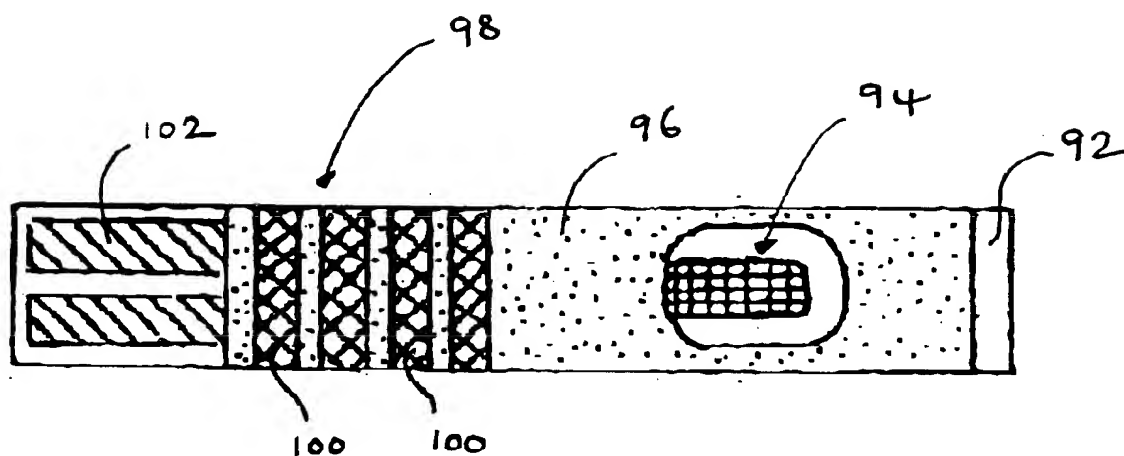


FIG. 11

8

